


Processing Record for this file:
(Make notes here unique for this file)

Loading from flight 140930a
Data taken from NOx CPU c:\data\CO


Flight used Dubey Manvendra's mixed gas 'standard'. The actual values of this standard have not yet been provided. On 140912, standard addition frequency changed from 1/30 min to 1/60 min. CO2 data file bifurcated. The two files were concatenated for processing. CO2 valve mistimed on ~14:50:50. A few seconds of cal deleted.

Ambient data appear valid.

Los Gatos ICOS CO/N2O/H2O Analyzer
Housekeeping

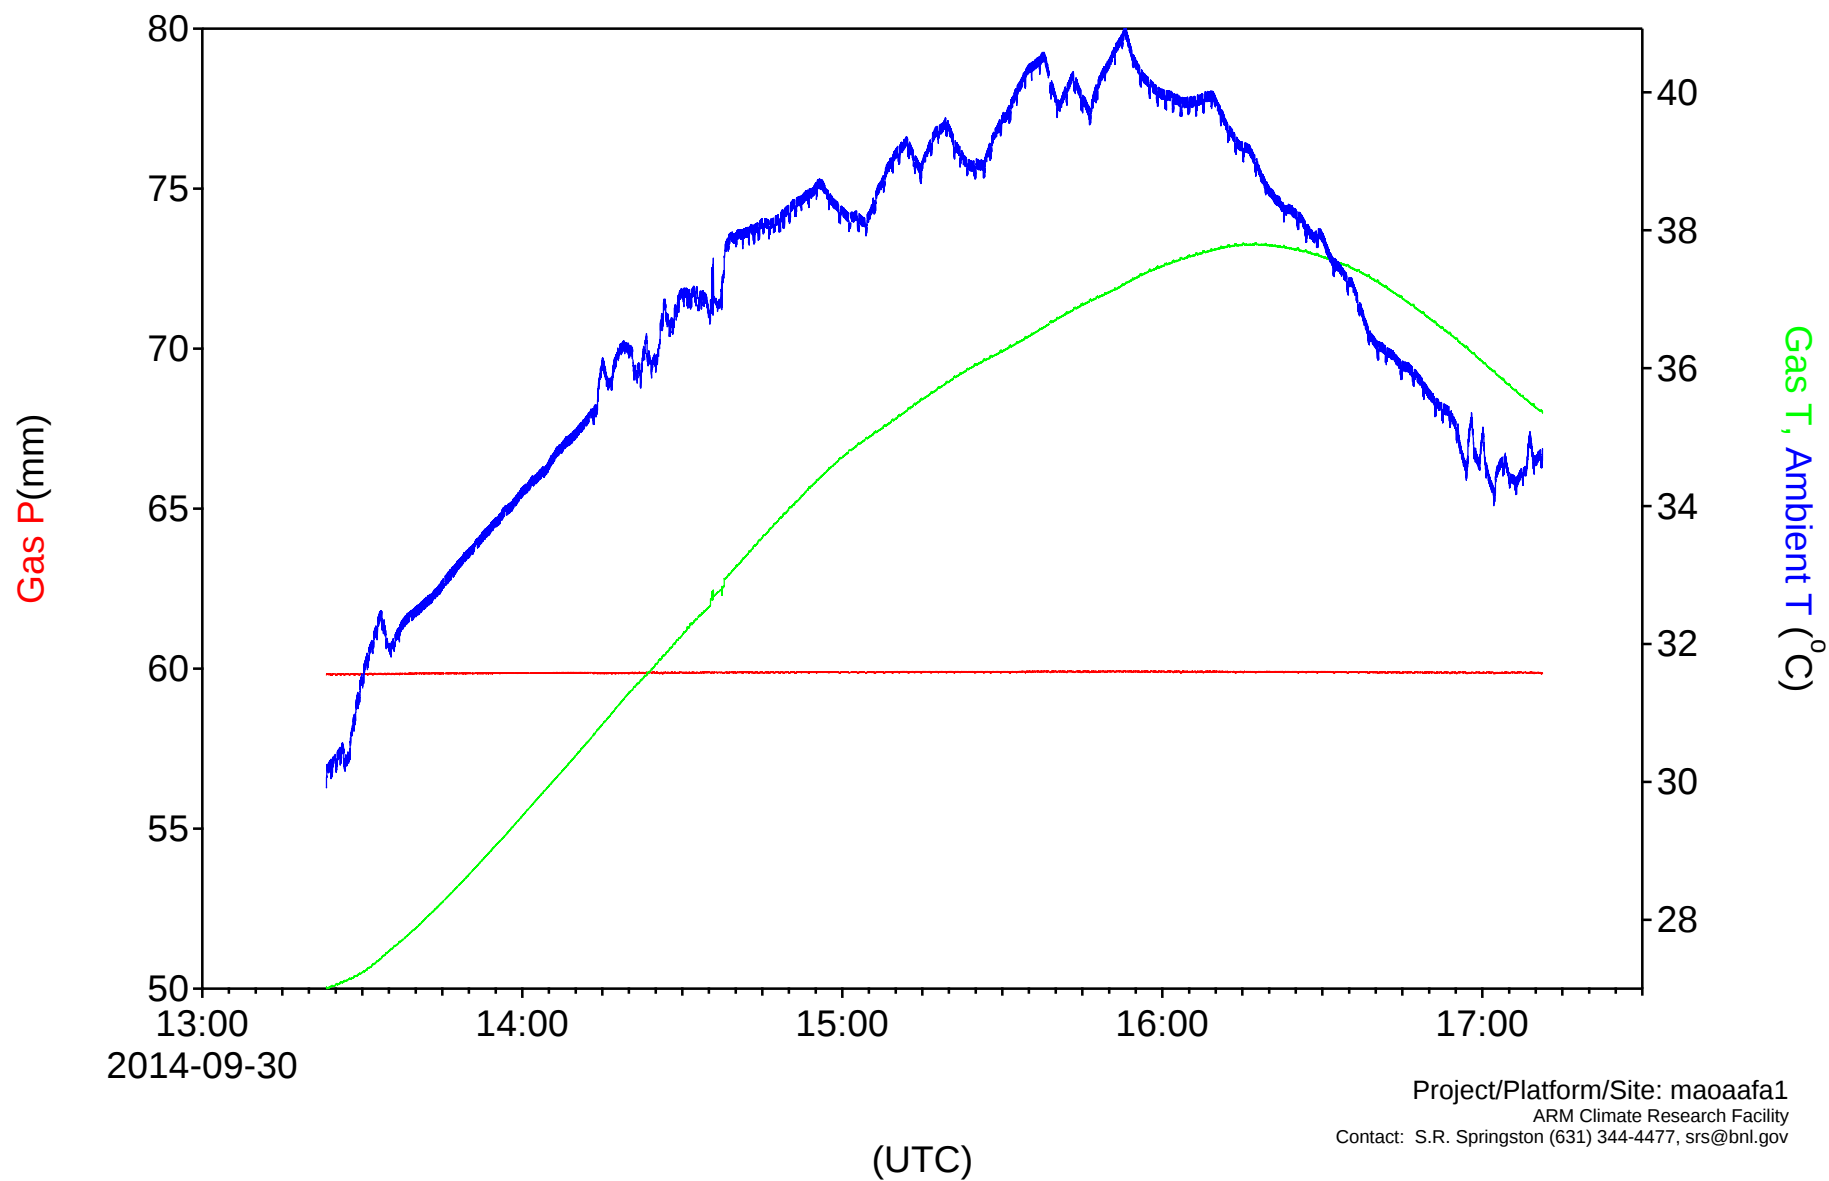


Los Gatos ICOS CO/N₂O/H₂O Analyzer Data

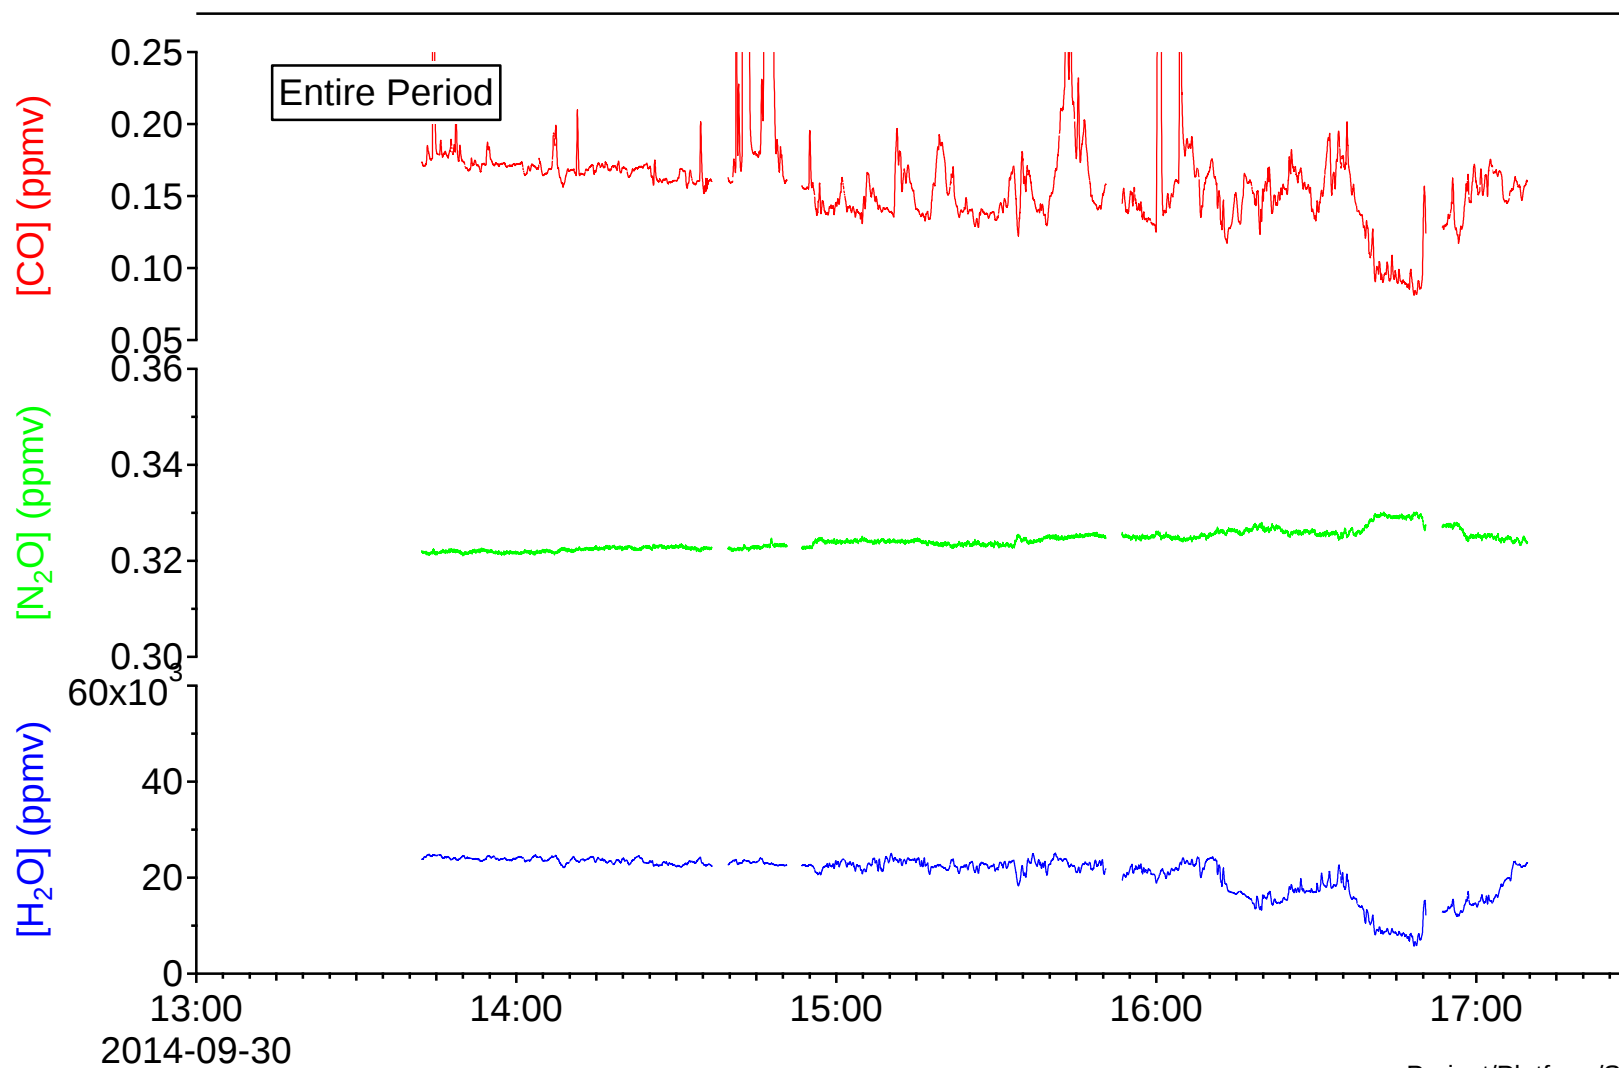

(UTC)

Project/Platform/Site: maoaafa1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov

Los Gatos ICOS CO/N2O/H2O Analyzer
Raw Data

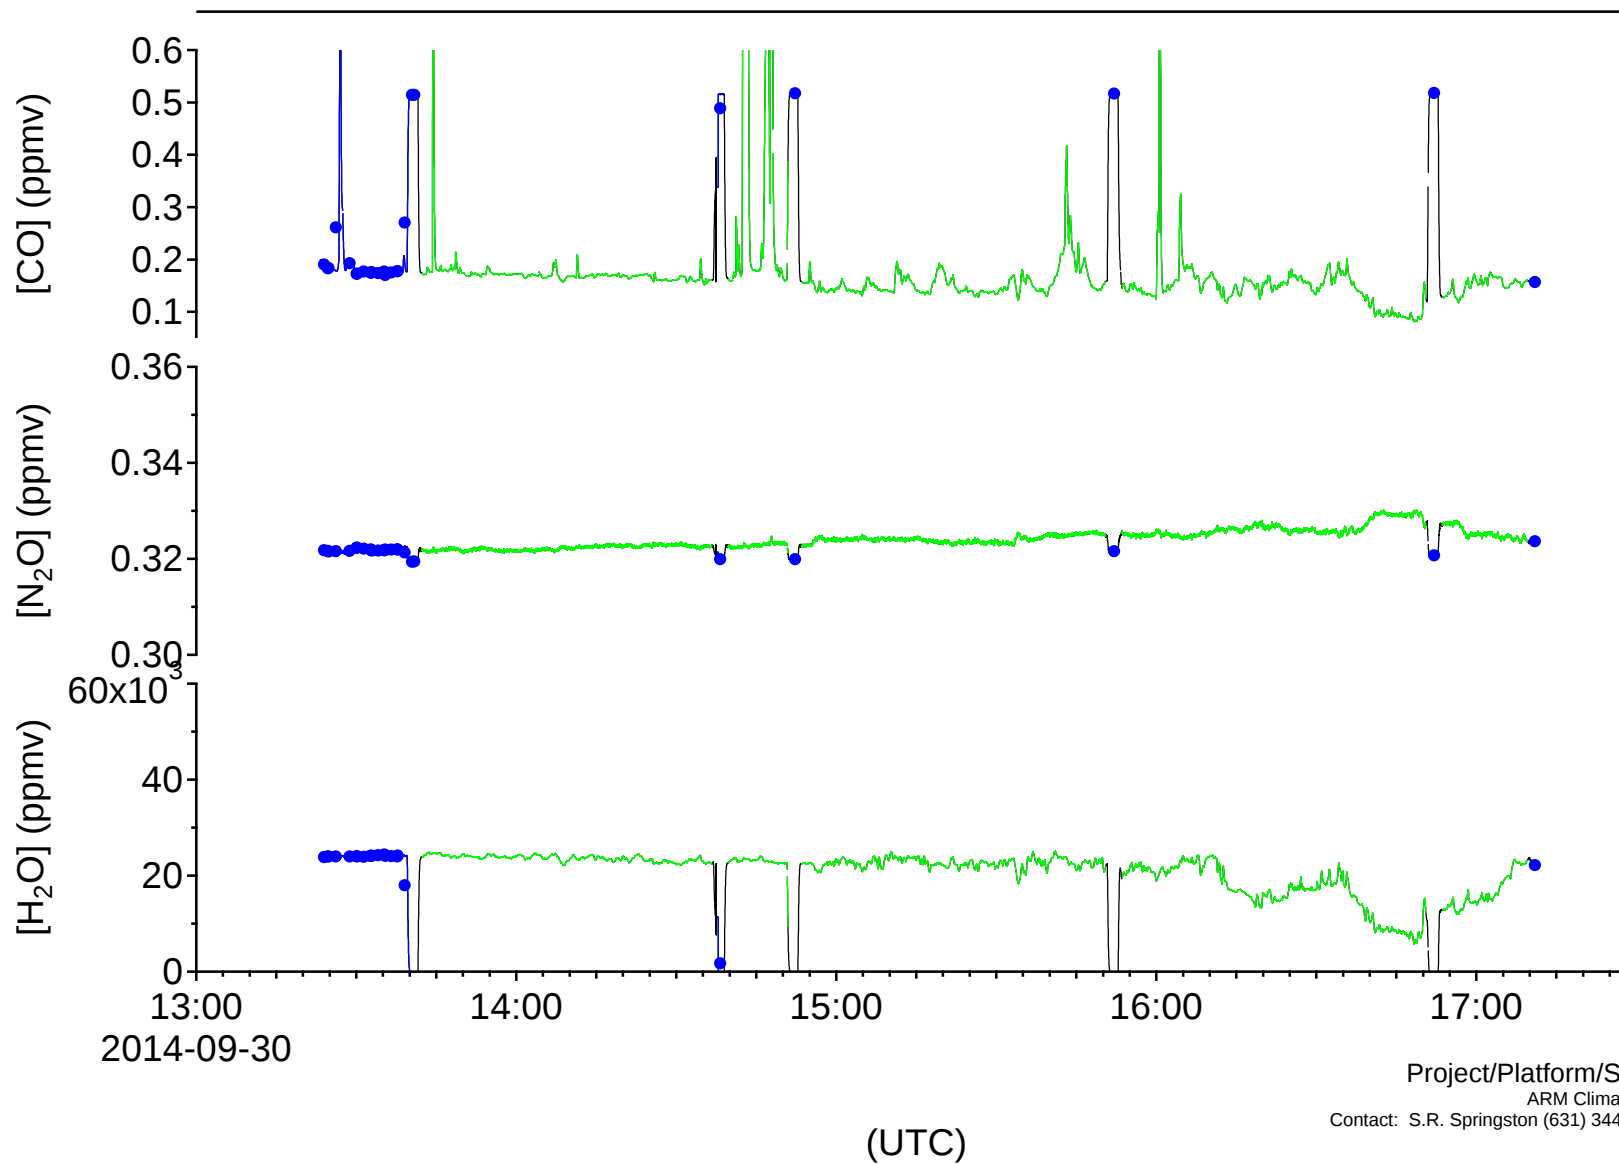

Project/Platform/Site: maoaafa1
ARM Climate Research Facility
Contact: S.R. Springston (631) 344-4477, srs@bnl.gov