


Processing Record for this file:  
(Make notes here unique for this file)

Loading from flight 140313a


Data taken from NOx CPU c:\data\ozone

Data appear normal. Units cells were removed and cleaned on 3/5/2014. This reduced noise greatly. Sample noise seems to have reappeared. Calibrations were ~20% low. This was not corrected in the reported data. It is expected that this was due to the internal pen-ray lamp source.


# TEI Model 49i UV Photometric Ozone Analyzer

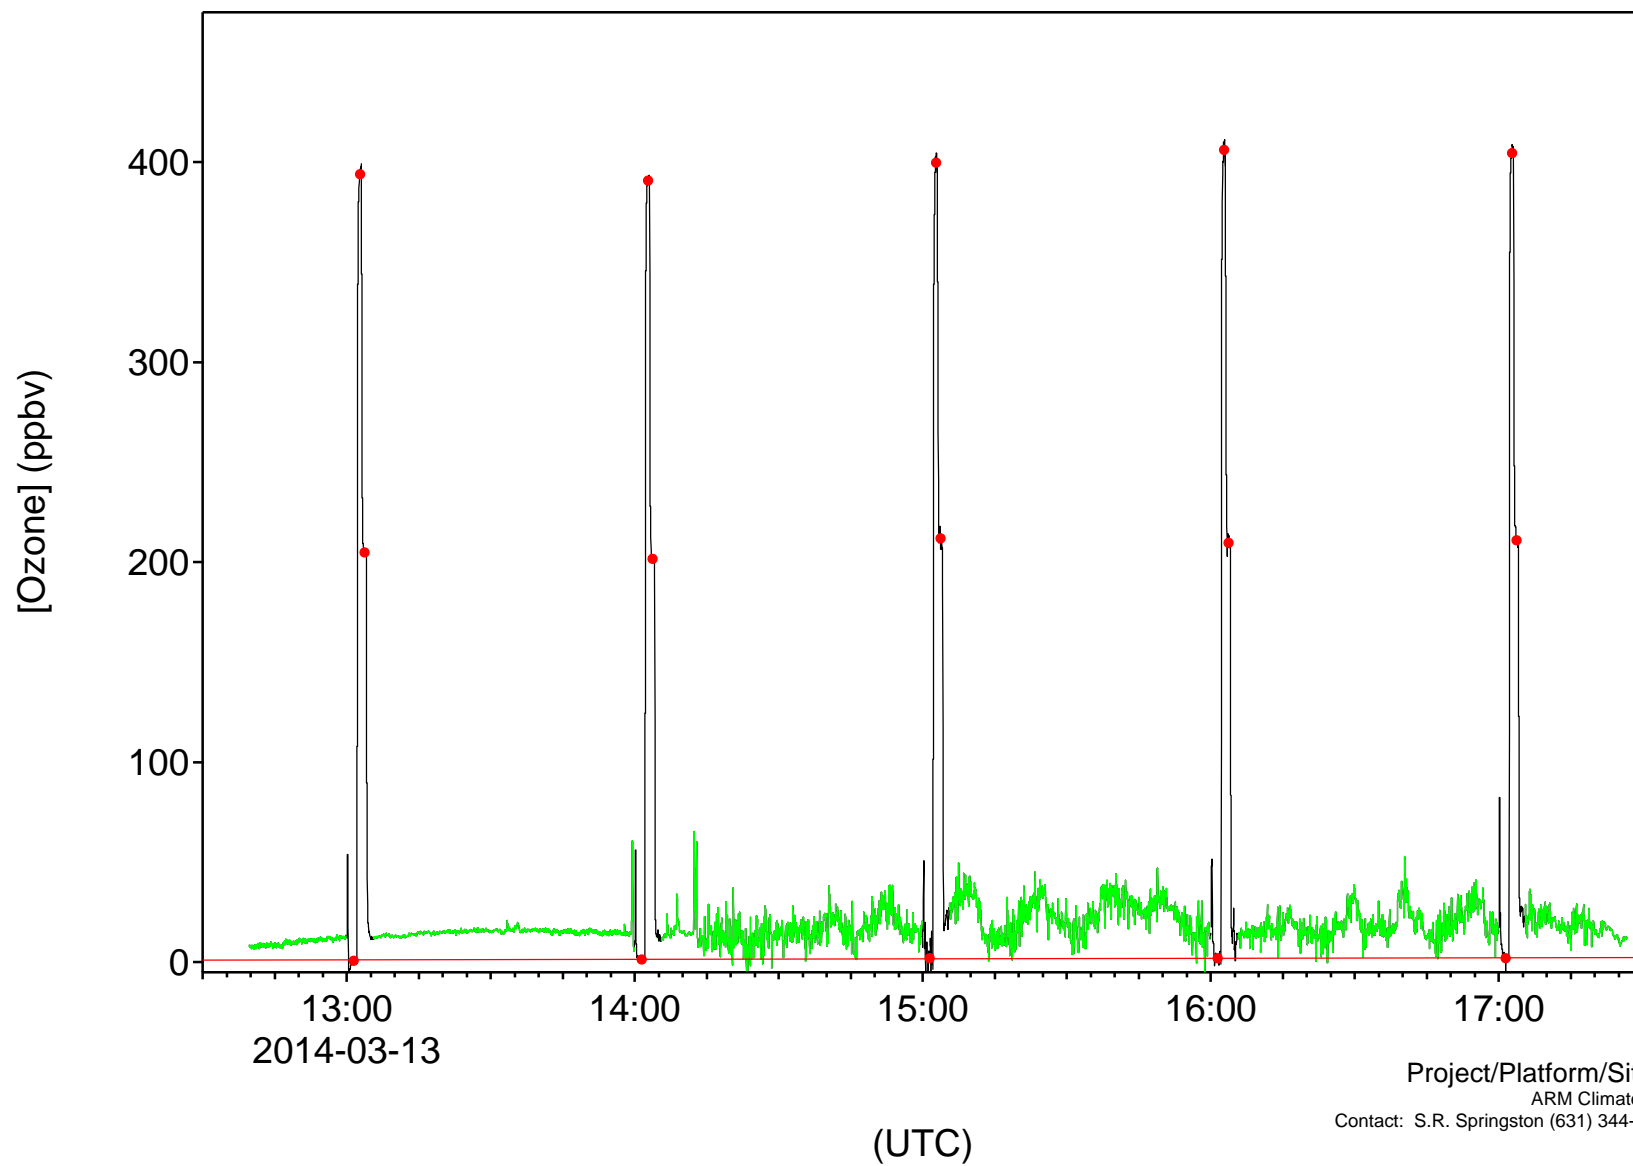

# TEI Model 49i UV Photometric Ozone Analyzer Housekeeping

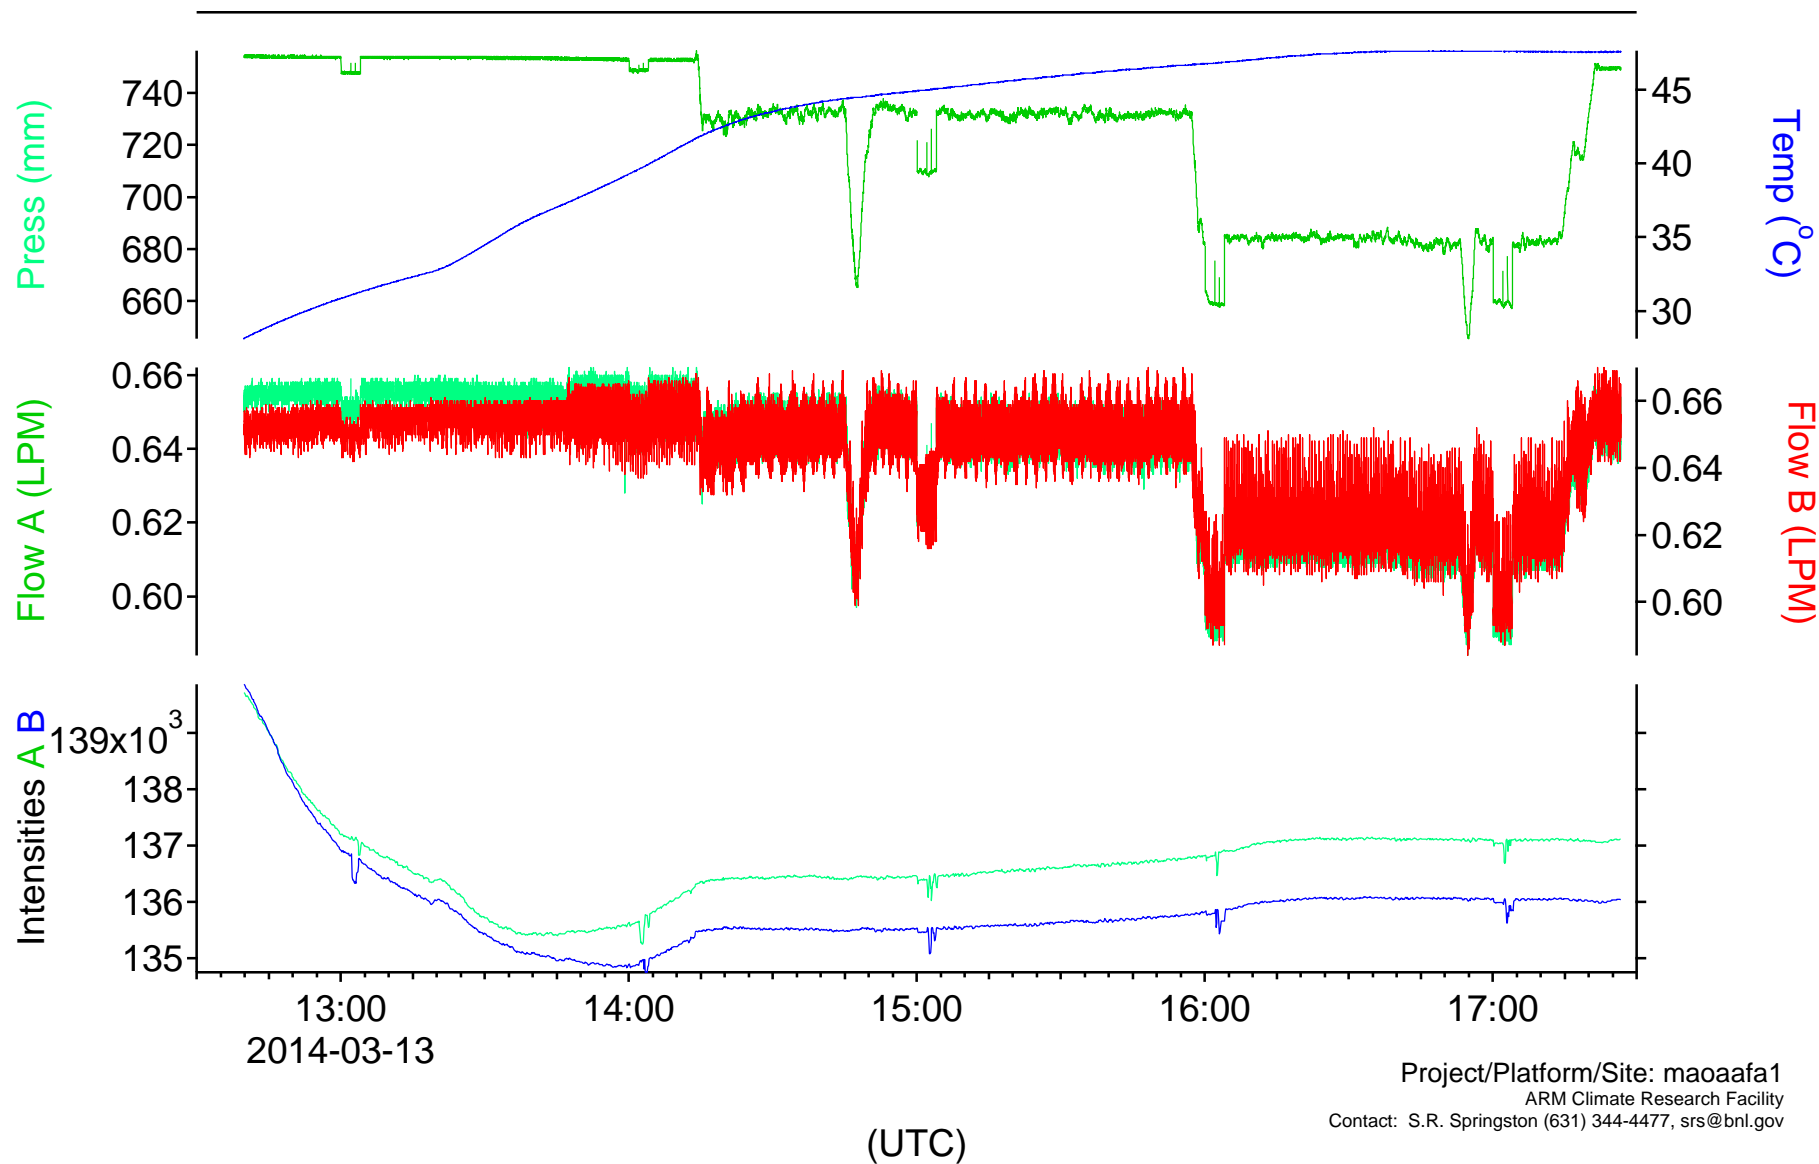

TEI Model 49i UV Photometric Ozone Analyzer  
Zero/Span Checks

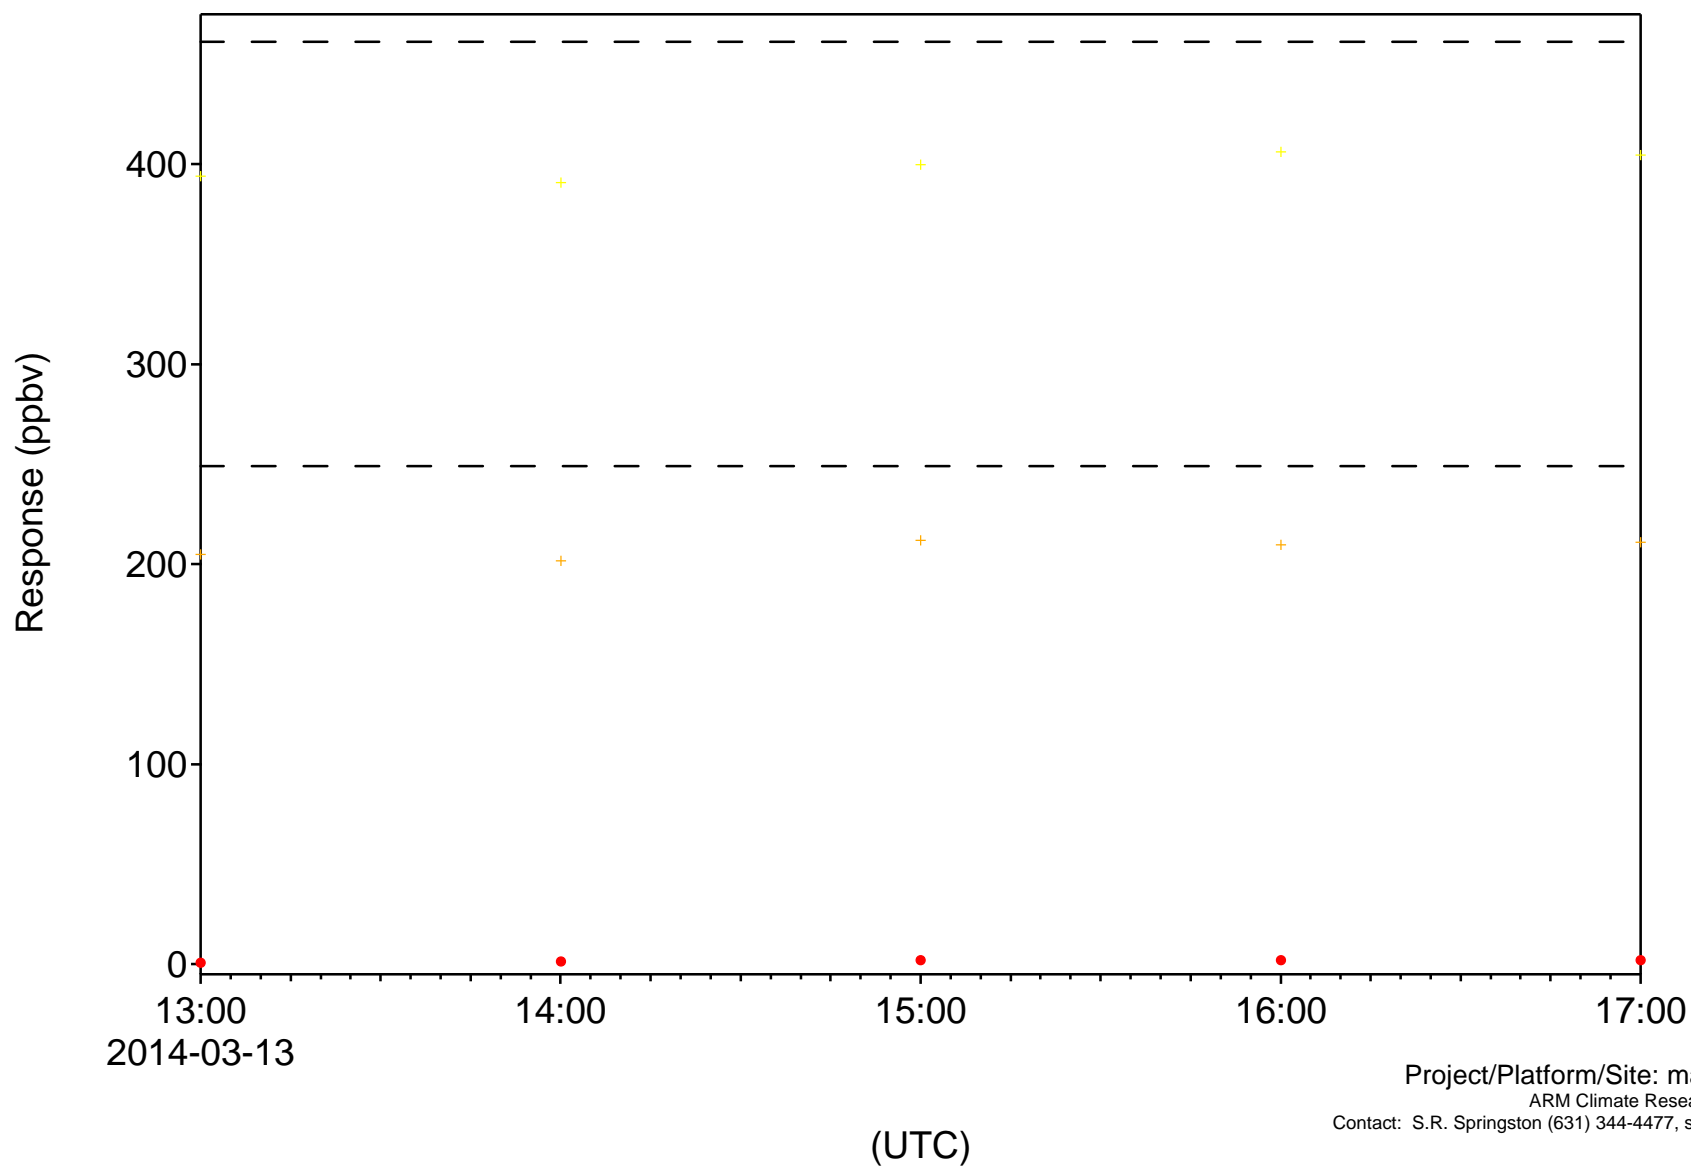

TEI Model 49i UV Photometric Ozone Analyzer  
Baseline Corrected

